



Design Configurations

Examples for Arthroscopy Punches

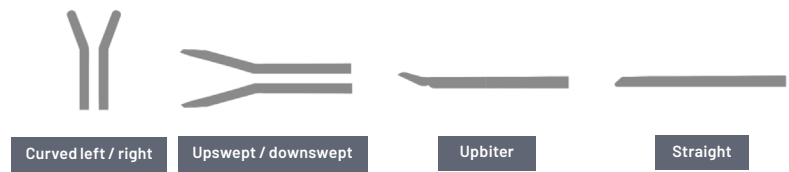

Posterior Punches

Ordering Information

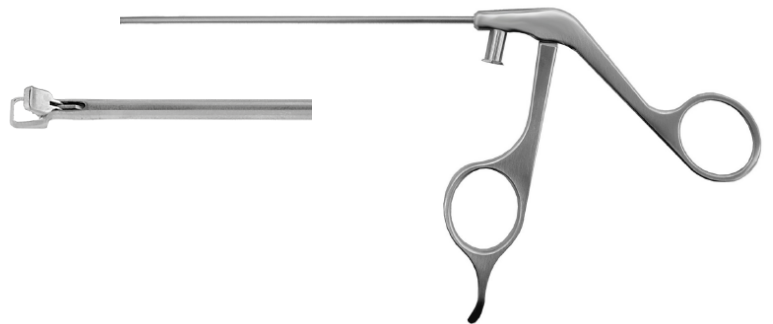

Punch serrated, large Ø 3.5mm, posterior, straight

17-4157

Punch serrated, large Ø 3.5mm, posterior, 7° upwards bent

17-4157-07

Punch serrated, large Ø 3.5mm, posterior, 15° downwards bent

17-4157-15

Punch serrated, medium Ø 3.5mm, posterior, 15° right bent


17-4157-L15

Punch serrated, medium Ø 3.5mm, posterior, 15° left bent

17-4157-R15

Scissor Punch

Ordering Information

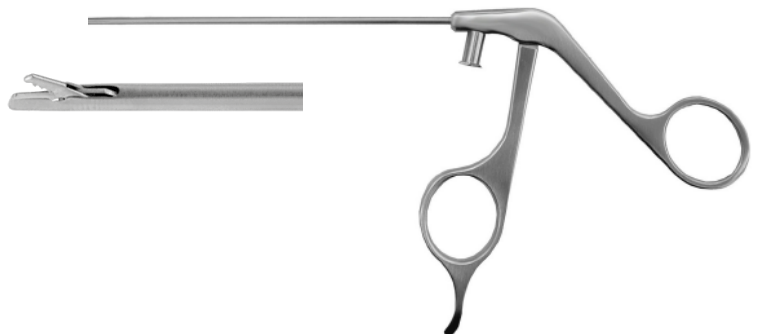


Scissors punch (SLENDER) Ø 3.5mm, straight

17-4185

Grasping Forceps

Ordering Information

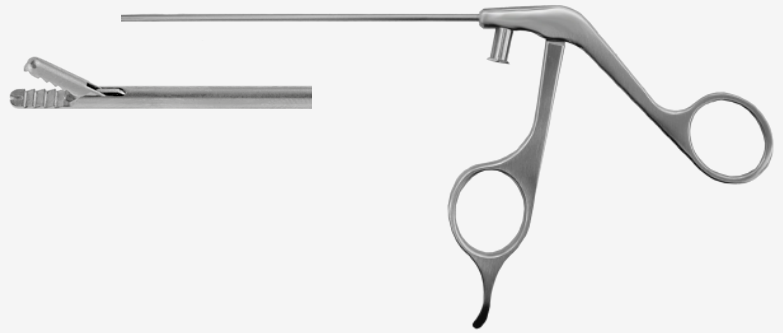

Grasper Ø 3.5mm with 1x2 teeth


17-4193

Grasper Ø 4.5mm with 1x2 teeth

17-4393

Alligator Graspers

Ordering Information

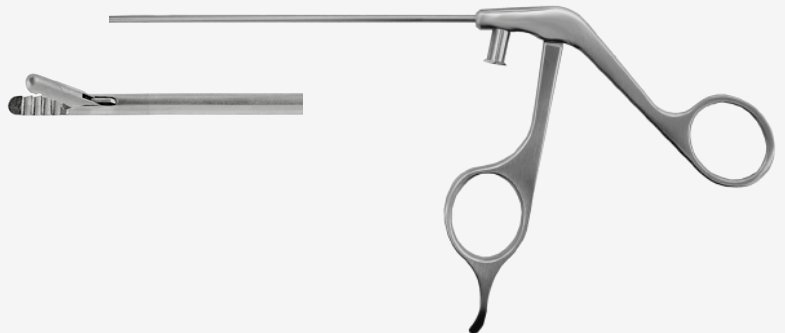


Alligator Grasper, Ø 3.5mm, straight

17-4191

Alligator Grasper, Ø 4.5mm, straight

17-4391

Hook Scissors

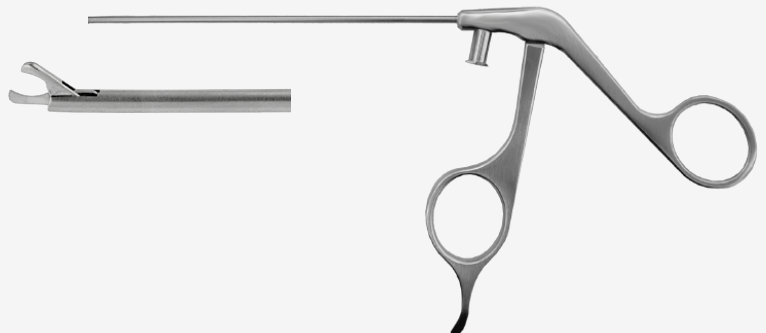

Hookscissors, Ø 3.5mm, 30° right bent

17-4180-R30

Graduated Probe

Ordering Information

Probe graduated, Ø 2.5mm

17-1802S



Banana Knife

Ordering Information

Banana knife, toothed

17-1807S



Smillie Knife

Ordering Information

Smillie knife, Ø 3.5mm

17-1810DK





www.ackermannsurgical.com



Ackermann Instrumente GmbH
Eisenbahnstrasse 65-67
78604 Rietheim-Weilheim, Germany

Revision 04/22